



# **IGFBP-2 Elisa**

***KAPME05***

---

**LOT** : 110301/1



# IGFBP-2-ELISA

Enzyme Immunoassay for the Quantitative Determination of  
Insulin-like Growth Factor Binding Protein-2

KAPME05

*IN VITRO DIAGNOSTIC USE*

en

DIAsource ImmunoAssays S.A. - Rue du Bosquet 2, B-1348 Louvain-la-Neuve, Belgium - Tel: +32 10 84 99 11 - Fax : +32 10 84 99 90

## TABLE OF CONTENTS

TECHNICAL FEATURES	2
INTENDED USE	2
CLINICAL IMPLICATIONS	2
INTRODUCTION	2
PHYSIOLOGICAL MEANING	2
MATERIALS	2
Materials Provided	2
Materials not Provided	3
WARNING AND PRECAUTIONS	3
METHODOLOGY	3
Principle	3
Sample Preparation and Storage	3
Technical hints	3
ASSAY PROCEDURE	4
EVALUATION OF RESULTS	4
Establishing the Calibration Curve:	4
PERFORMANCE CHARACTERISTICS	5
EXPECTED VALUES	6
LIMITATION	8
REFERENCES	8
SUMMARY OF THE ASSAY	9

## TECHNICAL FEATURES

Measures total IGFBP-2 concentration in serum, plasma and in other human body fluids  
Single standards with **2; 10; 20; 40 and 80 ng/ml**  
Total Incubation time only **1.75** hours  
2 Control Sera are provided for quality control purposes according GLP  
Ready-to-use Antibody Conjugate  
No sample extraction needed  
Microtiterplate separately break apart

## INTENDED USE

Measurement of human IGFBP-2 in human serum, EDTA-plasma, cerebrospinal fluid, breast milk, amniotic fluid, saliva and in cell culture medium.

## CLINICAL IMPLICATIONS

The IGFBP-2 concentration is age-dependent in blood (3).  
Normal values for healthy individuals (1.5 to > 70 years) were evaluated for this assay.  
Supplementary parameter to IGFBP-3 in the diagnosis of growth disorders (IGFBP-2/IGFBP-3 ratio), IGFBP-2 is an inhibitor of growth hormone action (3,4).  
Progression-dependent tumor marker in leukaemia (5), astrocytic CNS tumors (6,7), prostate- (8), suprarenal cortex-(9)-, hepatocellular (10) and other carcinomas.  
Anti-aging parameter: IGFBP-2 as a marker of physiological functionality (20).

## INTRODUCTION

Insulin-like growth factors (IGFs) regulate the proliferation, differentiation, apoptose, cell adhesion and metabolism in various tissues and cell types. The IGF-I, which is produced mainly in liver under the influence of growth hormone (GH), regulates as hormone the linear growth of the bones and the process of sexual maturity, while IGF-II is mainly a growth factor of fetal tissue (11-13). The biological actions of IGF over the IGF-Type-I receptor are modulated variably through the IGF binding proteins (IGFBP-1 to-6) (14). IGFBP-2 is, after IGFBP-3, the second most frequent IGFBP in the human blood. IGFs, especially tumor typical pro-IGF-forms and hormones regulate the expression of IGFBP-2, GH effect is thereby inhibiting. At cellular level IGFBP-2 seems to stimulate the proliferation and dissemination of solid tumors via an IGF-independent mechanism (15,16).

## PHYSIOLOGICAL MEANING

IGFBP-2 is a unglycosylated polypeptide of 31.3 kDa, which forms binary IGF-complexes and shows no circadian rhythm in the circulation. The serum concentration of IGFBP-2 increases in fasting, after major surgery and after trauma, but the increasing of the concentration is most intensive in malignant diseases. The correlation of the IGFBP-2 level to the degree of progression is a striking feature in various tumor types as is the normalization of the IGFBP-serum levels after remission (5-10). During the GH-therapy, e.g. in short stature and in GH-abuse (doping) the IGFBP-2 level decreases. In Trisomy 18 IGFBP-2 in maternal serum is decreased and IGFBP-1 is increased; therefore the ratio IGFBP-2 /IGFBP-1 is a marker for this chromosome abnormality (17).

## MATERIALS

### Materials Provided

- 1) 

TIT
-----

**Microtiter plate**, ready for use: **Microtiter plate** with 96 wells, divided up in 12 strips with 8 wells separately breakable, coated with anti-IGFBP-2 antibody and packed in a laminate bag.
  
- 2) 

CAL	N
-----	---

**Calibrators 1-5**, lyophilized: contain recombinant IGFBP-2: Calibrator values are between 2 - 80 ng/ml (2, 10, 20, 40, 80 ng/ml) IGFBP-2 and have to be reconstituted with **750 µl Dilution Buffer** each.
  
- 3) 

CONTROL	N
---------	---

**2 Controls**, lyophilized: Contains human serum and has to be reconstituted with **100 µl Dilution Buffer**. The exact concentration of IGFBP-2 is given on the vial label.
  
- 4) 

DIL	BUF
-----	-----

**Dilution Buffer**, 50 ml, ready for use.
  
- 5) 

Ab	BIOT
SAV	HRP

**Antibody-Conjugate**, 12 ml, ready for use, contains a mixture of biotinylated anti-IGFBP-2 antibody and HRP (Horseradish Peroxidase)-labelled Streptavidin. Use 100 µl/well in the assay.
  
- 6) 

WASH	SOLN	CONC
------	------	------

**Washing Buffer**, 50 ml, 20-fold concentrated: The **Washing Buffer** has to be diluted 1:20 with distilled water or demineralised water before use (e.g. add the complete contents of the flask (50 ml) into a graduated flask and fill up with A.dest. to 1000 ml). Please dilute only according to requirements. The diluted washing buffer is stable for 4 weeks at 2-8°C. It has to be at room temperature for usage !
  
- 7) 

CHROM	TMB
-------	-----

**TMB-Substrate Solution** 12 ml, ready for use, horseradish-peroxidase-(HRP)-substrate, stabilised H<sub>2</sub>O<sub>2</sub> Tetramethylbencidine.
  
- 8) 

STOP	SOLN
------	------

**Stopping Solution**, 0.2 M sulphuric acid, 12 ml, ready for use. *Caution Acid !*
  
- 9) **Sealing tape** for covering of the microtiter plate, 2 x

## Materials not Provided

- Precision pipettes (100 and 200µl) Micropipettes and multichannel pipettes with disposable plastic tips
- Distilled or Deionized water for dilution of the washing buffer
- Micropipettes and multichannel pipettes with disposable plastic tips
- Vortex-mixer
- Device to aspirate the calibrators and the samples from the wells (recommended because of the potential danger of infection by human samples)
- Plate washer and plate shaker ( $\geq 350$  rpm) (recommended)
- Calibrated Microplate reader ("ELISA-Reader") with filter for 450/620nm wavelength
- Foil welding device for laminate bags (recommended)
- Timer (120 min. range)
- Reservoirs (disposable)

## WARNING AND PRECAUTIONS

The kit should not be used beyond the expiration date on the kit label.

All reagents are for in vitro use only!

In conducting the assay, follow strictly the test protocol. The acquisition, possession and use of the kit are subject to the regulations of the national regulatory authorities.

Reagents with different lot numbers should not be mixed.

Reagents contain as preservative Proclin 950 (containing 0.009025% of 2-methyl-4-isothiazolin-3-one) and Kathon CG (containing 0.001615% of the mixture 5-chloro-2-methyl-4-isothiazolin-3-one and 2-methyl-4-isothiazolin-3-one). They can cause sensitisation by skin contact. (R 43 and S 26-36/37/39-45).

### First aid procedures:

*Skin contact:* Wash affected area thoroughly with water. Discard contaminated cloths and shoes.

*Eye contact:* In case of contact with eyes, rinse immediately with plenty of water at least 15 minutes. In order to assure an effectual rinsing spread the eyelids.

*Ingestion:* If swallowed, wash out mouth thoroughly with water. Immediately see a physician. The Stop Solution provided is an acid solution. Avoid direct contact. Wear eye, hand, face and clothing protection when using this material.

The handling of potentially infectious material must comply with the following guidelines:

Do not eat, drink or smoke in these areas.

Never pipette the materials with the mouth.

Spilled material must be wiped off immediately and should become disinfected. Clean contaminated areas and equipment with a suitable detergent.

## METHODOLOGY

### Principle

The DIAsource IGFBP-2 KAPME05 Elisa kit is a so-called Sandwich-Assay using two specific and high affinity antibodies. The IGFBP-2 in the samples binds to the first antibody coated on the microtiter plate. In the following step the second specific anti-IGFBP-2-Antibody binds in turn to the immobilised IGFBP-2. The second antibody is biotinylated and will be applied in a mixture with a Streptavidin-Peroxidase-Enzyme Conjugate. In the closing substrate reaction the turn of the colour will be catalysed quantitatively depending on the IGFBP-2-level of the samples.

### Sample Preparation and Storage

Serum and plasma samples as well as cell culture medium, breast milk, amniotic fluid, cerebrospinal fluid and saliva are applicable.

The blood sample for serum preparation should be gained according to standardized venipuncture procedure. The samples should be stored without anticoagulation reagents. Hemolytic reactions have to be avoided. The blood has to be allowed to clot and after complete clotting, serum is separated by centrifugation.

Blood samples may be taken at any time of the day.

Storage at RT max. 2 days

Storage at  $-20^{\circ}\text{C}$  max. 2 years

Are not allowed to have more than 10 freeze/thaw cycles.

### Sample preparation

Samples have to be diluted 1:10-30-fold with Dilution Buffer.

For clinical purposes we recommend a standard dilution of **1:21**.

### Suggestion for dilution protocol:

Mix 15 µl serum manually or with the aid of a dilutor with 300 µl Dilution Buffer (1:21). Use 2 x 100 µl of this dilution in the assay or pipette 100 µl buffer in wells and add 5 µl serum.

IGFBP-2 concentrations may be completely different in body fluids of human origin other than serum or cell culture supernatant (s. Table 5).

### Technical hints

The assay has to be conducted strictly according the test protocol herein.

Reagents with different lot numbers cannot be mixed.

### Calibrators and Controls

For the reconstitution of the lyophilised components (calibrators 1-5 and Control Sera), the kit Dilution Buffer has to be used. It is recommended to keep reconstituted reagents at room temperature for 15 minutes and then to mix them thoroughly but gently (no foam !) with a Vortex mixer.

The reconstituted calibrator and controls can be stored for 2 months at  $-20^{\circ}\text{C}$ . Repeated freeze/thaw cycles have to be avoided.

The Microtiterplate and all reagents are stable until the expiry date if stored in the dark at  $2-8^{\circ}\text{C}$  (see label). Store the unused seal stripes of the microtiterplate together with the desiccant at  $2-8^{\circ}\text{C}$ .

Bring all reagents to room temperature ( $20 - 25^{\circ}\text{C}$ ) before use. Possible precipitations in the buffers have to be resolved before usage by mixing and / or warming.

The required volume of washing buffer is prepared by 1:20 dilution of the provided 20fold concentrate with deionised water. The diluted washing buffer is stable for 4 weeks at 2-8°C. It has to be at room temperature for usage!  
 For reconstitution of lyophilized components the kit **Dilution Buffer** should be used. It is recommended to keep reconstituted reagents at room temperature for 15 minutes and then to mix them thoroughly but gently (no foam should result), with a Vortex mixer.  
 The reconstituted standard and controls can be stored for 2 month at -20°C..Avoid repeated freeze-thaw cycles.  
 Room temperature incubation means: incubation at 20 - 25°C.

## ASSAY PROCEDURE

All determinations (Calibrators, Control Sera and samples) should be assayed in duplicate. For optimal results, accurate pipetting and adherence to the protocol are recommended.

When performing the assay, the **Calibrators 1-5 and Control Serum** should be pipetted as fast as possible (e.g., 15 Minutes). Antibody-Conjugate and the **Substrate solution** should be added to the plate in the same order and the same time interval as the samples. **Stop Solution** should be added to the plate in the same order as the **Substrate Solution**.

- 1) Add **100 µl** Dilution Buffer to the first wells (blank). Subsequently, add **100µl** of each Calibrator or diluted **Control (1 & 2)** or diluted **Sample** to the following wells.
- 2) Cover the wells with sealing tape and incubate the plate for **1 hour** shaking at room temperature at  $\geq 350$  rpm.
- 3) After incubation aspirate the contents of the wells into a disinfectant (risk of infection!) and wash the wells 3 times with **250 µl** of **Washing Buffer** / well respectively. The **Washing Buffer** should incubate at least for **15 seconds**/well.
- 4) Following the last washing step pipette **100µl** of the **Antibody-Conjugate** in each well. and incubate the plate for **30 Minutes** shaking at **room temperature at  $\geq 350$  rpm**.
- 5) After incubation wash the wells 3 times with **Washing Buffer** as described above.
- 6) Pipette **100 µl** of the **TMB-substrate** solution in each well.
- 7) Incubate the plate for **15 minutes** in the dark at **room temperature**.
- 8) Stop the reaction by adding **100 µl** of **Stopping Solution** to all the wells.
- 9) Measure the absorbance within **30 minutes** at **450 nm** (reference filter:  $\geq 590$  nm).

## EVALUATION OF RESULTS

### Establishing the Calibration Curve:

The calibrators provided contain the following concentrations of IGFBP-2:

Standard	A	B	C	D	E
Ng/ml	2	10	20	40	80

- 1) Calculate the mean absorbance (MA) value for the blank from the duplicated determination (well A1/A2).
- 2) Subtract the mean absorbance (MA) of the blank from the mean absorbance of all other values.
- 3) Plot the calibrators concentrations 1-5 on the x-axis versus the mean value of the absorbance of the calibrators on the y-axis. Read the concentration of each control and sample by interpolation on the calibration curve.
- 4) Recommendation: Calculation of calibration curve and sample concentrations should be done by using a computer programme, because the standard curve is in general best described by non-linear regression, a higher-grade polynomial or four parametric logistic (4-PL) curve fit are in general suited for the evaluation.
- 5) The IGFBP-2 concentration of the diluted sample or the diluted control sera 1&2 in ng/ml is calculated in this way, the IGFBP-2 concentration of the **undiluted sample** and of 1 & 2 is calculated **by multiplication** with the respective dilution factor.

The exemplary shown calibration curve in Fig.1 **cannot be used** for calculation of your test results. You have to establish a calibration curve for each test you conduct!

Exemplary calculation of the IGFBP-2 concentration of undiluted sample:

Measured extinction of your sample	0.37
Measured extinction of the blank	0.06


Your **measurement program** will calculate the IGFBP-2 concentration of the diluted sample automatically by using the difference (0.31) of sample and blank for the calculation. You only have to determine the most suitable curve fit (here: polynomial 3<sup>rd</sup> degree).

In this exemplary case the following equation is solved by the program to calculate the IGFBP-2 concentration in the sample:

$$0.31 = -0.0012048 + 0.039581x + 5.1788 \cdot 10^{-0,005} \cdot x^2 - 1.8929x \cdot 10^{-0,06} \cdot x^3$$

$$7.93 = x$$

if the dilution factor (**1:21**) is taken into account the IGFBP-2 concentration of the undiluted sample is  $7.93 \times 21 = 166.55$  ng/ml

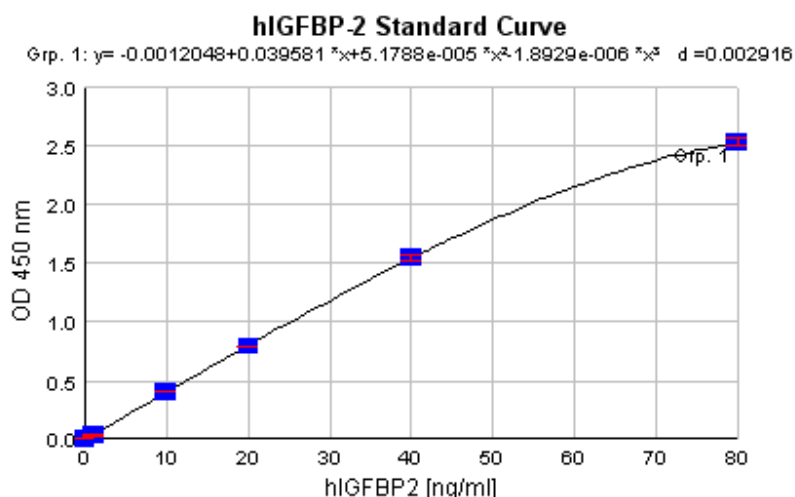

**Fig. 1: Exemplary Calibration Curve** with a polynomial 3<sup>rd</sup> degree as curve fit.

## PERFORMANCE CHARACTERISTICS

### Standards

The Standards of the IGFBP-2 Elisa KAPME05 are prepared from **human IGFBP-2** in concentrations of 2, 10, 20, 40 and 80 ng/ml.

### Sensitivity

The analytical sensitivity of the assay yields 0.2 ng/ml (2x SD of zero calibrator)

### Specificity

This assay is specific for human IGFBP-2, only low degree of cross reactions was found with dog, horse, donkey, cat and goat. No cross-reactivity was with pig, bovine, rabbit, mouse, chicken, rat, guinea pig, sheep.

There is no cross-reactivity with IGFBP-1 nor IGFBP-3

### Interference

Interference of bilirubin and triglycerides was tested by adding different amounts of these substances to human serum containing IGFBP-2. For comparison the same amount of buffer without any substance was also added to the serum. Table 1 demonstrates that neither bilirubin nor triglycerides exert any influence on the measurement of IGFBP-2 in human serum.

**Table 1: Interference**

Bilirubin		Triglycerides	
[µg/ml]	% of control	[mg/ml]	% of control
25	95.07	12.5	100.79
50	92.80	25	101.01
100	93.83	50	103.65
200	88.15	100	101.34

### Recovery

Recombinant IGFBP-2 was added in three different concentration to human serum. The IGFBP-2 concentration was measured and the mean relative recovery in comparison to buffer was 108%. Some exemplary data are shown in table 2.

**Table 2: Recovery of recombinant human IGFBP-2 in Serum**

NIBSC IGFBP-2 [ng/ml]	+1000 ng/ml	+500 ng/ml	+100 ng/ml	Mean [ng/ml]
% Recovery	100,00	112,00	114,00	108,67

### Reproducibility and Precision

The inter- and intra assay coefficients of variability are below 10%. Exemplary determinations are shown in table 3 and 4.

**Table 3 : Interassay-Variation**

Sample1 (ng/ml)	137	159	152
Sample 2 (ng/ml)	672	697	688
Sample 3 (ng/ml)	928	929	956

**Table 4: Intra-Assay-Variation**

Sample 1 ng/ml	322	375	298	305	318	311	320	325	302	301	305	317
Sample 2 ng/ml	612	609	616	648	594	597	620	613	617	611	636	698

**Table 5: Linearity of the sample dilution:**

Dilution	Serum 1 (ng/ml)	Serum 2 (ng/ml)	Cerebrospinal fluid (ng/ml)	Amniotic fluid (ng/ml)
1:10	938	582	426	Not determined
1:20	1061	673	428	460
1:40	1055	719	379	483
1:80	1004	691	318	431
1:160	952	668	426	415

**EXPECTED VALUES**

The IGFBP-2 concentration in serum is depended on age (Table 8) and on Body Mass Index (BMI; Table 7). For data collection of these reference values IGFBP-2 levels were determined in serum of over 400 normal children and adults (see table 8 figure 2); (3).

Please see the expected values of IGFBP-2 levels in other human body fluids than serum and in cell culture medium in the table 6.

**Table 6: Expected values of IGFBP-2 in body fluids of human origin and in cell culture supernatants:**

Sample	Expected Value (ng/ml)
serum	[ 100 - 1000 ]
liquor	[ 100 - 300 ]
amniotic fluid	[ 200 - 10000 ]
seminal plasma	[ 5000 - 15000 ]
breast milk	[1500-3000]
cell culture supernatants	[ 5 - 300 ]


**Table 7: BMI dependent reference values, adults between 20 and 80 years**

BMI [kg/m <sup>2</sup> ]	N	IGFBP-2 [ng/ml]		percentiles		
		mean	SD	5th	50th	95th
15	12	612	110	431	612	793
17,5	14	568	126	361	568	775
20	76	509	144	271	509	746
22,5	124	449	162	182	449	716
25	101	398	165	127	398	670
27,5	52	348	147	106	348	590
30	25	315	118	120	315	510
32,5	15	282	90	135	282	430
35	4	251	80	119	251	383
37,5	4	220	71	104	220	336



**Table 8:** IGFBP-2 serum levels (in ng/ml) of > 400 healthy individuals. The normal range is given by the 5., 50. and 95. percentile for age classes.  
**Age-dependent normal range of serum IGFBP-2**

age (years)	5. percentile (ng/ml)	50. percentile (ng/ml)	95. percentile (ng/ml)
1	408	545	728
2	359	500	696
3	317	460	668
4	277	421	640
5	243	388	617
6	217	361	602
7	194	336	583
8	173	312	562
9	154	289	542
10	138	268	522
11	123	249	503
12	111	232	486
13	101	219	477
14	94	212	470
15	89	207	465
16	86	207	460
17	84	214	466
18	84	223	483
19	84	232	500
25	99	280	580
35	110	381	686
45	130	403	702
55	140	410	715
65	151	418	727
75	153	427	740
80	156	430	744

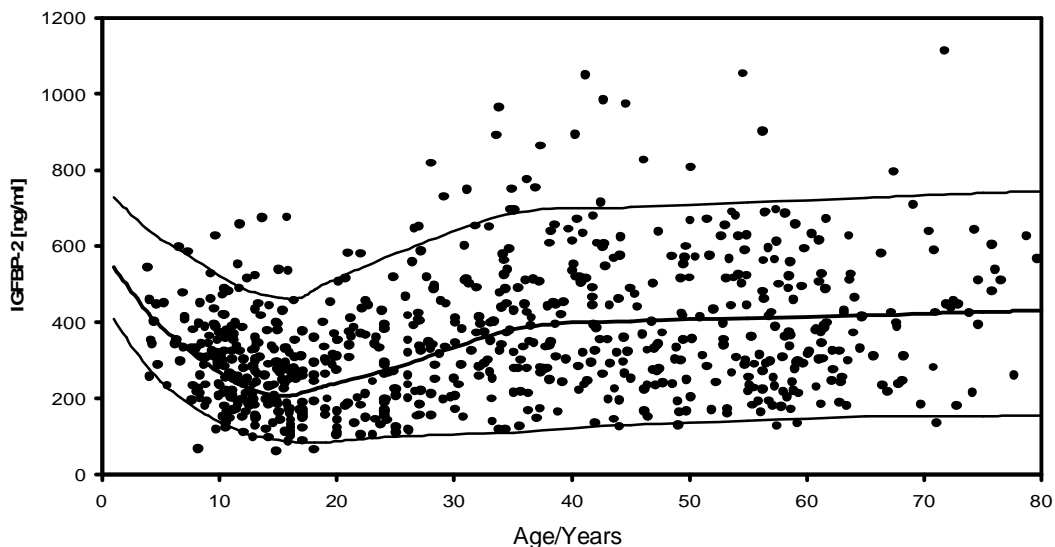

Assembled by Dr. R. Schweizer, Tübingen, Germany

#### LIMITATION

Deviation from the reference range can be expected especially in hypothyroidism, after major surgery, in polytrauma, in Diabetes mellitus (due to insulin therapy), in fasting and in malignant diseases.

#### REFERENCES

- Elmlinger MW, Wimmer K, Biemer E, Blum WF, Ranke MB, Dannecker GE, (1996) Insulin-like growth factor binding protein 2 is differentially expressed in leukaemic T- and B-cell lines. *Growth Regulation* 6, 152-157
- Hoeflich A, Nedbal S, Blum WF, Erhard M, Lahm H, Brem G, Kolb HJ, Wanke R, Wolf E. (2001) Growth inhibition in giant growth hormone transgenic mice by overexpression of insulin-like growth factor-binding protein-2. *Endocrinology* 142:1889-98
- Ranke MB, Schweizer R, Elmlinger MW, Weber K, Binder G, Schwarze CP, Wollmann HA (2000) Significance of basal IGF-I, IGFBP-3 and IGFBP-2 measurements in the diagnostics of short stature in children. *Hormone Research* 54: 60-68
- Ranke MB, Schweizer R, Elmlinger MW, Weber K, Binder G, Schwarze CP, Wollmann HA (2001). Relevance of IGF-I, IGFBP-3, and IGFBP-2 measurements during GH treatment of GH-deficient and non-GH-deficient children and adolescents. *Hormone Research* 55: 115-124
- Crofton PM, Ahmed SF, Wade JC, Elmlinger MW, Ranke MB, Kelnar CJH, Wallace WHB (1999) Effects of a third intensification block of chemotherapy on bone and collagen turnover, insulin-like growth factor I, its binding proteins and short term growth in children with acute lymphoblastic leukemia. *European Journal of Cancer* 35: 960-967
- Muller HL, Oh Y, Lehrnbecher T, Blum WF, Rosenfeld RG. (1994) Insulin-like growth factor-binding protein-2 concentrations in cerebrospinal fluid and serum of children with malignant solid tumors or acute leukemia. *J Clin Endocrinol Metab.* 79: 428-34
- Martin W, Elmlinger, Martin H, Deininger, Burkhardt S, Schuett, Richard, Meyermann, Frank, Duffner, Ernst H, Grote, and Michael B, Ranke (2001) In vivo expression of the insulin-like growth factor binding protein-2 in human gliomas increases with the tumor grade. *Endocrinology* 142: 1652-1658
- Cohen P, Peehl DM, Stamey TA, Wilson KF, Clemmons DR, Rosenfeld RG (1993) Elevated levels of insulin-like growth factor-binding protein-2 in the serum of prostate cancer patients. *J Clin Endocrinol Metab.* 76: 1031-1035
- Boulle N, Baudin E, Gicquel C, Logie A, Bertherat J, Penfornis A, Bertagna X, Luton JP, Schlumberger M, Le Bouc Y. (2001) Evaluation of plasma insulin-like growth factor binding protein-2 as a marker for adrenocortical tumors. *Eur J Endocrinol.* 144: 29-36
- Ranke MB, Maier KP, Schweizer R, Stadler B, Schleicher s, Elmlinger MW, Flehmig B (2003), Pilot study of elevated levels of insulin-like growth factor-binding protein-2 as indicators of hepatocellular carcinoma. *Horm Res* 60:174-180
- Rosenfeld RG, Roberts CT Jr. (eds.) (1999) *The IGF system: Contemporary Endocrinology Series*; Humana Press
- Jones JI, Clemmons DR. (1995) Insulin-like growth factors and their binding proteins: biological actions. *Endocr Rev.* 16: 3-34
- Chard T (1994) Insulin-like growth factors and their binding proteins in normal and abnormal fetal growth. *Growth Reg* 4: 91-100
- Ranke MB, Elmlinger MW (1997) Functional role of insulin-like growth factor binding proteins. *Hormone Research* 48 (suppl 4): 9-15
- Elmlinger MW, Bell M, Schütt, BS, Langkamp M, Kutob E, Ranke MB (2001) Transactivation of the IGFBP-2 promoter in human tumor cell lines. *Molecular and Cellular Endocrinology* 175: 211-218
- Hoeflich A, Reisinger R, Lahm H, Kiess W, Blum WF, Kolb HJ, Weber MM, Wolf E. (2001) Insulin-like growth factor-binding protein 2 in tumorigenesis: protector or promoter? *Cancer Res.* 15: 8601-8610
- Miell JP, Langford KS, Jones JS, Noble P, Westwood M, White A, Nicolaides KH. (1997) The maternal insulin-like growth factor (IGF) and IGF-binding protein response to trisomic pregnancy during the first trimester: a possible diagnostic tool for trisomy 18 pregnancies. *J Clin Endocrinol Metab.* 82: 287-292

18. Elmlinger MW., Regine Grund, Michael Buck, Hartmut A Wollmann, Norman Feist, Matthias M. Weber, Christian C. Speer and Michael B. Ranke (1999). Limited proteolysis of the insulin-like growth factor binding protein (IGFBP)-2 by a specific serine protease activity in early breast milk. *Pediatric Research* 46: 76-81
19. Elmlinger MW, Michael S Sanatani, Mathias Bell, Günther E Dannecker, Michael B Ranke (1998) Elevated insulin-like growth factor (IGF) binding protein (IGFBP)-2 and IGFBP-4 expression of leukemic T-cells is affected by autocrine/paracrine IGF-II action but not by IGF type I receptor expression. *European Journal of Endocrinology* 138: 337-343
20. van den Beld, Blum W, Pols H, Grobbee D, Lamberts S (2003) Serum insulin-like growth factor binding protein-2 levels as an indicator of functional ability in elderly men. *European Journal of Endocrinology* 148: 627-634







#### SUMMARY OF THE ASSAY

Reagent:	Reconstitution:	dilution:
Calibrators 1-5	in 750 µl Dilution Buffer	
Control Serum 4 ( 1 & 2) <sup>o</sup>	in 100 µl Dilution Buffer	1:21 with Dilution Buffer
Washing Buffer		1:20 with Distilled water (e.g., add the complete contents of the flask (50 ml) into a graduated flask and fill with Distilled water to 1000 ml).
Sample Dilution: Serum samples should be diluted prior to measurement 1:10-30-fold with Dilution Buffer depending on the expected values. In general a dilution of 1:21 is appropriate. Use 2 x 100 µl of this dilution in the assay		

#### Assay Procedure for Double Determination

Pipette	Reagents	Position
100 µl	Dilution Buffer	A1/2
100 µl	Calibrator 1 ( 2 ng/ml)	B1/2
100 µl	Calibrator 2 (10 ng/ml)	C1/2
100 µl	Calibrator 3 (20 ng/ml)	D1/2
100 µl	Calibrator 4 (40 ng/ml)	E1/2
100 µl	Calibrator 5 (80 ng/ml)	F1/2
100 µl	Control Serum 1	G1/2
100 µl	Control Serum 2	H1/2
100 µl	Sample dilution	following wells
Cover the wells with the sealing tape.		
<b>Incubation: 1 h at RT, ≥ 350 rpm</b>		
3x 250 µl	Aspirate the contents of the wells and wash 3x with 250 µl Wash Buffer	each well
100 µl	Antibody-Conjugate	each well
<b>Incubation: 30 min at RT, ≥ 350 rpm</b>		
3x 250 µl	Aspirate the contents of the wells and wash 3x with 250 µl Wash Buffer	each well
100 µl	Substrate Solution	each well
<b>Incubation: 15 min in the Dark at RT</b>		
100 µl	Stopping Solution	each well
Measure the absorbance within 30 min at 450 nm with ≥ 590 nm as reference wavelength.		

Revision Date: 2011-03-01

	<b>Used symbols</b>
	Consult instructions for use
	Storage temperature
	Use by
<b>LOT</b>	Batch code
<b>REF</b>	Catalogue number
<b>CONTROL</b>	Control
<b>I V D</b>	In vitro diagnostic medical device
	Manufacturer
	Contains sufficient for <n> tests
WASH SOLN CONC	Wash solution concentrated
CAL 0	Zero calibrator
CAL N	Calibrator #
CONTROL N	Control #
Ag 1251	Tracer
Ab 1251	Tracer
Ag 1251 CONC	Tracer concentrated
Ab 1251 CONC	Tracer concentrated
	Tubes
INC BUF	Incubation buffer
ACETONITRILE	Acetonitrile
SERUM	Serum
DIL SPE	Specimen diluent
DIL BUF	Dilution buffer
ANTISERUM	Antiserum
IMMUNOADSORBENT	Immunoabsorbent
DIL CAL	Calibrator diluent
REC SOLN	Reconstitution solution
PEG	Polyethylene glycol
EXTR SOLN	Extraction solution
ELU SOLN	Elution solution
GEL	Bond Elut Silica cartridges
PRE SOLN	Pre-treatment solution
NEUTR SOLN	Neutralization solution
TRACEUR BUF	Tracer buffer
<b>µP</b>	Microtiterplate
Ab HRP	HRP Conjugate
Ag HRP	HRP Conjugate
Ab HRP CONC	HRP Conjugate concentrate
Ag HRP CONC	HRP Conjugate concentrate
CONJ BUF	Conjugate buffer
CHROM TMB CONC	Chromogenic TMB concentrate
CHROM TMB	Chromogenic TMB solution
SUB BUF	Substrate buffer
STOP SOLN	Stop solution
INC SER	Incubation serum
BUF	Buffer
Ab AP	AP Conjugate
SUB PNPP	Substrate PNPP
BIOT CONJ CONC	Biotin conjugate concentrate
AVID HRP CONC	Avidine HRP concentrate
ASS BUF	Assay buffer
Ab BIOT	Biotin conjugate
Ab	Specific Antibody
SAV HRP CONC	Streptavidin HRP concentrate
NSB	Non-specific binding
2nd Ab	2nd Antibody
ACID BUF	Acidification Buffer
DIST	Distributor