



# INSTRUCTION MANUAL

IVD

( April 01, 2014 )

# Medizym<sup>®</sup> anti-CCP Ref

- 96 determinations -

REF 3860



Enzyme immunoassay for the determination of IgG autoantibodies to cyclic citrullinated peptides (CCP) in human serum or plasma



**MEDIPAN GMBH**

Ludwig-Erhard-Ring 3

**15827 Dahlewitz / Berlin (Germany)**

...

Phone: +49(0)33 708 / 44 17 - 0

Fax: +49(0)33 708 / 44 17 - 25

info@medipan.de  
www.medipan.eu

## INTENDED USE

Medizym<sup>®</sup> anti-CCP Ref is used for the quantitative determination of IgG antibodies against cyclic citrullinated peptides (CCP) in human sera.

Rheumatoid Arthritis (RA) is most often diagnosed by the measurement of rheumatoid factors (RF). The rheumatoid factor is an antibody directed against the Fc-region of IgG. It appears mainly as IgM antibody but also as IgA or IgG subgroup.

Rheumatoid factors are present in sera of 70 - 80 % of patients suffering from rheumatoid arthritis. But it is not specific for RA since it will also be found in healthy persons. The incidence depends on the age: for young people it is 1 - 4 %, for older persons it may reach up to 25 %.

The advantage of CCP antibodies is a higher sensitivity and specificity for the diagnosis of rheumatoid arthritis in comparison to the rheumatoid factors alone. Anti-CCP is often found at a very early state of the disease and it has a high predictive value for development of the disease.

## PRINCIPLE of the TEST

Medizym<sup>®</sup> anti-CCP Ref is an enzyme immunoassay for the quantitative determination of IgG autoantibodies to cyclic citrullinated peptides (CCP) in human serum.

In the first step CCP AAb from the diluted sample (as well as from the calibrators and control) bind to cyclic citrullinated peptides coated on the microtiter plate. After an incubation of 60 minutes at room temperature (RT) unbound components are removed by washing.

In a next step bound antibodies reacts with the added anti-human-IgG horseradish peroxidase (HRP) complex. Excessive conjugate is removed after 30 minutes at RT by another washing step.

HRP converts the colorless substrate TMB added into a blue product. The enzyme reaction is stopped by adding an acid solution after 15 minutes at RT. The color changes from blue to yellow. The absorbance of the resulting product is measured at 450 / 620 nm within 30 minutes. The obtained OD is direct proportional to the amount of bound antibodies.

## PATIENT SAMPLES

### Specimen collection and storage

Blood is taken by venipuncture. After clotting, the serum is separated by centrifugation. Do not use lipaemic or grossly hemolytic serum samples.

The samples may be kept at 2 - 8 °C up to three days. Long-term storage requires - 20 °C.

Repeated freezing and thawing should be avoided. For multiple use, aliquot samples and keep them at - 20 °C.

### FU symbols non-radioactive assays MEDIPAN GMBH

IVD	In vitro diagnostic device	CE	EC Declaration of Conformity
REF	Catalogue number	LOT	Batch code
	Expiry date		Manufactured by
	Consult accompanying documents		Consult operating instruction
	Store at		Biological risk
MP	Coated microtiterplate (96 wells)	DIL	Sample diluent
WASHB	Wash buffer	SUB	Substrate
CAL	Calibrators	CONJ	Conjugate
STOP	Stop solution	CONTROL	Control serum

## TEST COMPONENTS for 96 DETERMINATIONS

<b>A</b> <b>MP</b>	<b>Microtiter plate</b> 12 breakable strips, 8 wells per strip coated with synthetic peptides with citrulline residues	<b>1</b> vacuum sealed with desiccant
<b>B</b> <b>WASHB</b>	<b>Concentrated wash buffer</b> 10 fold, sufficient for 1000 ml	<b>100 ml</b> concentrate white capped
<b>D</b> <b>CONJ</b>	<b>Anti human IgG (sheep) Horseradish -peroxidase (HRP) complex</b>	<b>15 ml</b> ready for use red capped
<b>E</b> <b>SUB</b>	<b>Substrate</b> (3,3',5,5'-Tetramethylbenzidin)	<b>15 ml</b> ready for use blue capped
<b>F</b> <b>STOP</b>	<b>Stop solution</b> (0.25 M sulfuric acid)	<b>15 ml</b> ready for use yellow capped
<b>G</b> <b>DIL</b>	<b>Sample diluent</b>	<b>100 ml</b> ready for use black capped
<b>C I</b> <b>CONTROL</b>	<b>Negative Control</b> concentration: see leaflet <span style="border: 1px solid black; padding: 2px;">-</span>	<b>1 ml</b> ready for use green capped
<b>C II</b> <b>CONTROL</b>	<b>Positive Control</b> concentration: see leaflet <span style="border: 1px solid black; padding: 2px;">+</span>	<b>1 ml</b> ready for use red capped
<b>1 - 5</b> <b>CAL</b>	<b>Calibrators:</b> concentrations see leaflet	<b>5 vials</b> <b>1 ml</b> each, ready for use white capped

### Materials required

- Precision pipettes 5 - 1000 µl
- Multi-channel pipette
- Disposable pipette tips
- 8 channel wash comb or microplate washer
- Micro plate reader with optical filters for 450 nm and 620 or 690 nm
- Graduated cylinders
- Distilled or de-ionized water
- Absorbent paper or paper towel
- tubes (2 ml) for sample dilution
- foil

### Size and storage

Medizym® anti-CCP has been designed for 96 determinations. This is sufficient for the analysis of 42 unknown samples as well as for calibrators and control serum assayed in duplicates.

The expiry date of each component is reported on its respective label, that one of the complete kit on the box label.

Upon receipt, all components of the Medizym® anti-CCP Ref have to be kept at 2 - 8 °C, preferably in the original kit box.

### Preparation before use

Allow samples to reach room temperature prior to assay. Take care to agitate serum samples gently in order to ensure homogeneity.

Note: Patients samples have to be diluted 1 + 100  
e.g. 5 µl sample + 500 µl sample diluent (G)

#### Please, handle the following components carefully:

- A** Allow the sealed microplate to reach room temperature before opening for at least 30 minutes. Unused wells should be stored refrigerated and protected from moisture in the original bag. Carefully resealed it can be used for 8 weeks.
- B** Prepare a sufficient amount of washing solution by diluting the concentrated wash buffer (B) 1 + 9 with distilled or de-ionized water. For example, dilute 50 ml of the concentrate with 450 ml of distilled water. B should be free of crystals before dilution, otherwise dissolve by warming up to max. 37 °C. The diluted washing solution can be stored at 2 - 8 °C up to 30 days.
- D** The anti-human IgG-HRP solution is stable up to 8 weeks at 2 - 8 °C after opening.
- E** Avoid exposure of substrate solution (E) to light.

## ASSAYS PROCEDURE

- Duplicates are recommended.

1. Pipette into the corresponding wells according to assay scheme
    - **100 µl** calibrators (1 - 5)
    - **100 µl** diluted patient sample and controls (C I, C II).
  2. Cover the plate and incubate for **60 min** at RT (18 - 25 °C).
  3. Aspirate or "flick out" by striking the wells sharply onto absorbent paper to remove any residual droplets. Wash **3 times** with **300 µl** washing solution (diluted from B) with 5 seconds soaking time each.
  4. Add **100 µl** of anti-human IgG - HRP (D) to each well.
  5. Cover the plate and incubate for **30 min** at RT.
  6. Aspirate or "flick out" by striking the wells sharply onto absorbent paper to remove any residual droplets. Wash **3 times** with **300 µl** washing solution (diluted from B) with 5 seconds soaking time each.
  7. Add **100 µl** substrate solution (E) to each well and shake shortly.
  8. Incubate for **15 min** in the **dark** at RT.
  9. Add **100 µl** stop solution (F) to each well.
- Avoid any time shift during pipetting the samples and reagents.**
10. Read the optical density (OD) **at 450 nm** versus **620 or 690 nm** **within 30 min** after adding the stop solution.

Please note that the washing procedure is crucial. Insufficient washing will result to poor precision and falsely elevated OD readings. After each washing step any residual fluid has to be removed completely.

The plate should be shortly shaken after each pipetting step.

Please make sure to avoid any contamination by germs or fungi or any other substances since this would lead to incorrect results.

## DATA PROCESSING

The standard curve is established by plotting the mean OD-values of the calibrators 1 - 5 on the ordinate, y-axis, versus their respective CCP-Ab-concentrations on the abscissa, x-axis (log scale).

The CCP Ab concentrations of the controls and the unknown diluted samples are directly read off in U/ml from the measured OD<sub>450</sub> values. There is no further correction for the dilution necessary.

Medizym® anti-CCP Ref may be used also with Computer Assisted Analysis with software able to use spline smoothing fitting.

We recommend 4 parameter fit.

## TYPICAL EXAMPLE


Do not use for evaluation!



Sample	OD (a) 450 nm	OD (b) 450 nm	OD (mean)	U/ml
Calibrator 1	0.037	0.043	0.040	1
Calibrator 2	0.304	0.285	0.295	20
Calibrator 3	0.514	0.551	0.533	40
Calibrator 4	1.771	1.589	1.680	400
Calibrator 5	2.631	2.284	2.458	2000
Patient 1	1.024	1.019	1.022	103

## STANDARD CURVE

Typical example

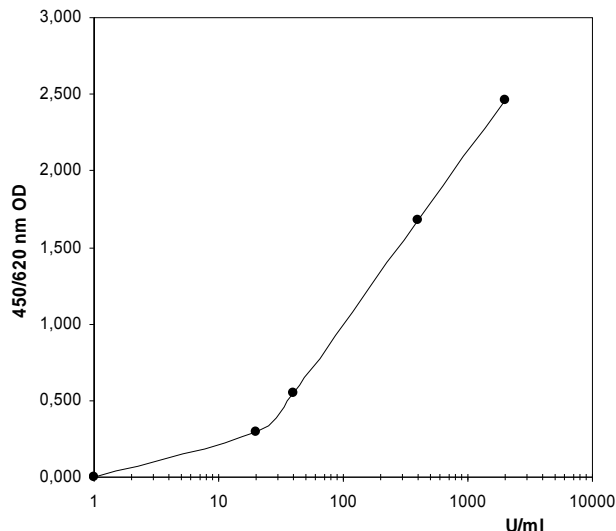

### Criteria of validation

Specimens with an OD higher than Standard 5 should be diluted further by the sample diluent and the concentration of CCP antibodies should be calculated by the applied dilution factor.

## REFERENCE VALUES

Medizym® anti-CCP Ref	
negative	< 30 U/ml
positive	≥ 30 U/ml

It is recommended that each laboratory establishes its own normal and pathological reference ranges for serum anti-CCP antibodies levels as usually done for other diagnostic parameters, too. Therefore, the abovementioned reference values provide only a guide.

## CHARACTERISTIC ASSAY DATA

### Calibration

The Medizym® anti-CCP Ref is artificially calibrated and concentrations of anti-CCP are therefore expressed in U/ml. Those units show a constant factor (1 : 12) to the WHO Reference standard W1066 for rheumatoid arthritis.

### Linearity

On the basis of the heterogeneous nature of the autoantibody population and in view of epitope specificity and affinity of the autoantibodies the theoretical values expected by dilution with anti-CCP free human serum most often correspond with the measured concentrations.

### Specificity and sensitivity

The results available show a clinical sensitivity of 79 % at a specificity of 97 % for the diagnosis of rheumatoid arthritis.

### Detection limit

The analytical sensitivity (lower detection limit, 0 + 3 SD) was established to be 1.2 U/ml.

The functional sensitivity was measured as 20 % of inter-assay CV at about 2 U/ml.

### Intra - and Inter-assay variation

Intra-Assay (n = 20)			Inter-Assay (n = 5 x 10)		
Sample no.	Mean Concentration (U/ml)	CV (%)	Sample no.	Mean Concentration (U/ml)	CV (%)
1	21	10.3	1	27	8.6
2	218	4.8	2	226	6.0
3	1150	2.4	3	1240	4.1

## LIMITATIONS of the METHOD

Healthy individuals should be tested negative by using the Medizym® anti-CCP Ref. However, CCP autoantibodies may also be present in apparently healthy persons.

Any clinical diagnosis should not be based on the results of in vitro diagnostic method alone. Physicians are supposed to consider all clinical and laboratory findings possible to state a diagnosis.

# Medizym<sup>®</sup> anti-CCP Ref

## ASSAY SCHEME

Bring all reagents to room temperature. Gently mix all reagents to ensure homogeneity.  
Dilute all samples 1 + 100 (v + v) by sample diluent (G).

Step	Activity	Material	CAL	CI / C II	Diluted patient samples 1, 2 etc.
1	Pipette	Samples	100 µl	100 µl	100 µl
2	Incubate	Plate (A)	1 hour at RT (18 - 25 °C)		
3	Aspirate or decant	put sharply onto absorbent tissue			
	Pipette	Washing solution made from B	3 x 300 µl 5 seconds each	3 x 300 µl 5 seconds each	3 x 300 µl 5 seconds each
4	Pipette	Anti-human IgG HRP (D)	100 µl	100 µl	100 µl
5	Incubate	Plate (A)	30 min at RT (18 - 25 °C)		
6	Aspirate or decant	put sharply onto absorbent tissue			
	Pipette	Washing solution made from B	3 x 300 µl 5 seconds each	3 x 300 µl 5 seconds each	3 x 300 µl 5 seconds each
7	Pipette	Substrate (E)	100 µl	100 µl	100 µl
8	Incubate	Plate (A)	15 min at RT (18 - 25 °C) in the dark		
9	Pipette and mix	Stop solution (F)	100 µl	100 µl	100 µl
10	Measure OD	at 450 nm versus 620 nm (or 690 nm) within 30 min			

## SAFETY PRECAUTIONS

- **This kit is for in vitro use only.** Follow the working instructions carefully. This instruction manual is valid only for the present kit with the given composition. An exchange of single components is not in agreement with CE regulations.
- The expiration dates stated on the respective labels are to be observed. The same relates to the stability stated for reconstituted reagents.
- Do not use or mix reagents from different lots.
- Do not use reagents from other manufacturers.
- Avoid time shift during pipetting of reagents.
- All reagents should be kept at 2 - 8 °C before use in the original shipping container.
- Some of the reagents contain small amounts ( $\leq 1\%$  v/v) Neolone M10 as a preservatives. They must not be swallowed or allowed to come into contact with skin or mucosa.
- Source materials derived from human body fluids or organs used in the preparation of this kit were tested and found negative for HBsAg and HIV as well as for HCV antibodies. However, no known test guarantees the absence of such viral agents. Therefore, handle all components and all patient samples as if potentially hazardous.
- Since the kit contains potentially hazardous materials, the following precautions should be observed:
  - Do not smoke, eat or drink while handling kit material,
  - Always use protective gloves,
  - Never pipette material by mouth,
  - Wipe up spills promptly, washing the affected surface thoroughly with a decontaminant.
- In any case GLP should be applied with all general and individual regulations to the use of this kit.